

FIG. 1

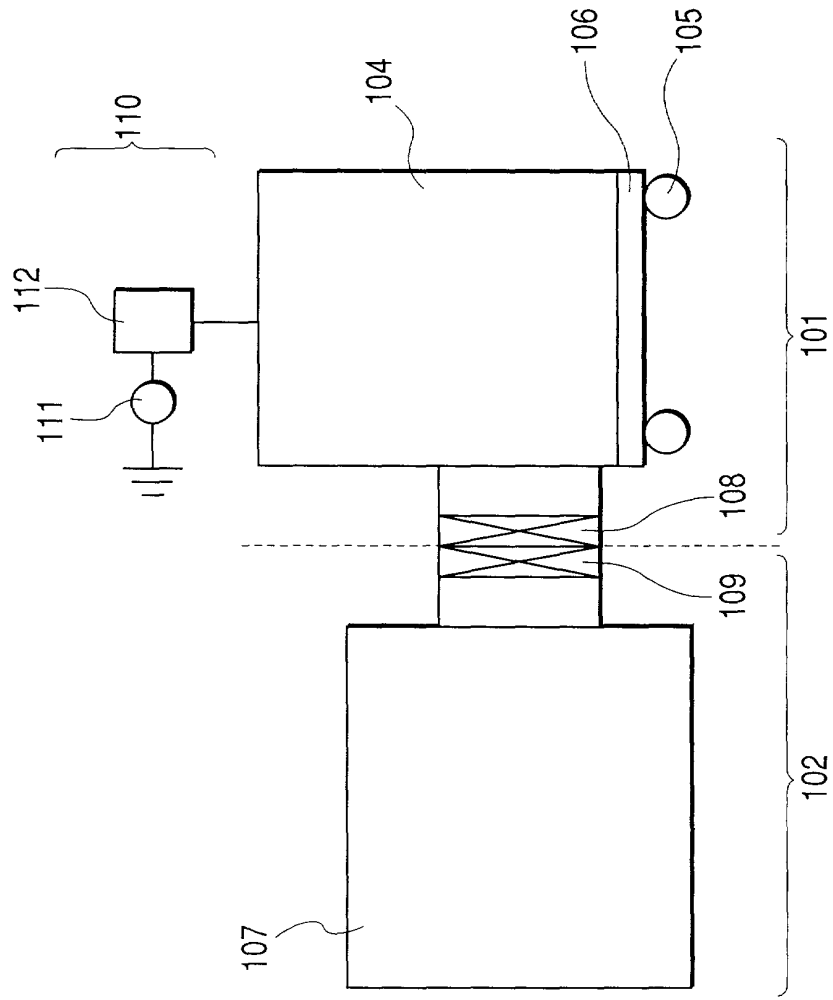


FIG. 2

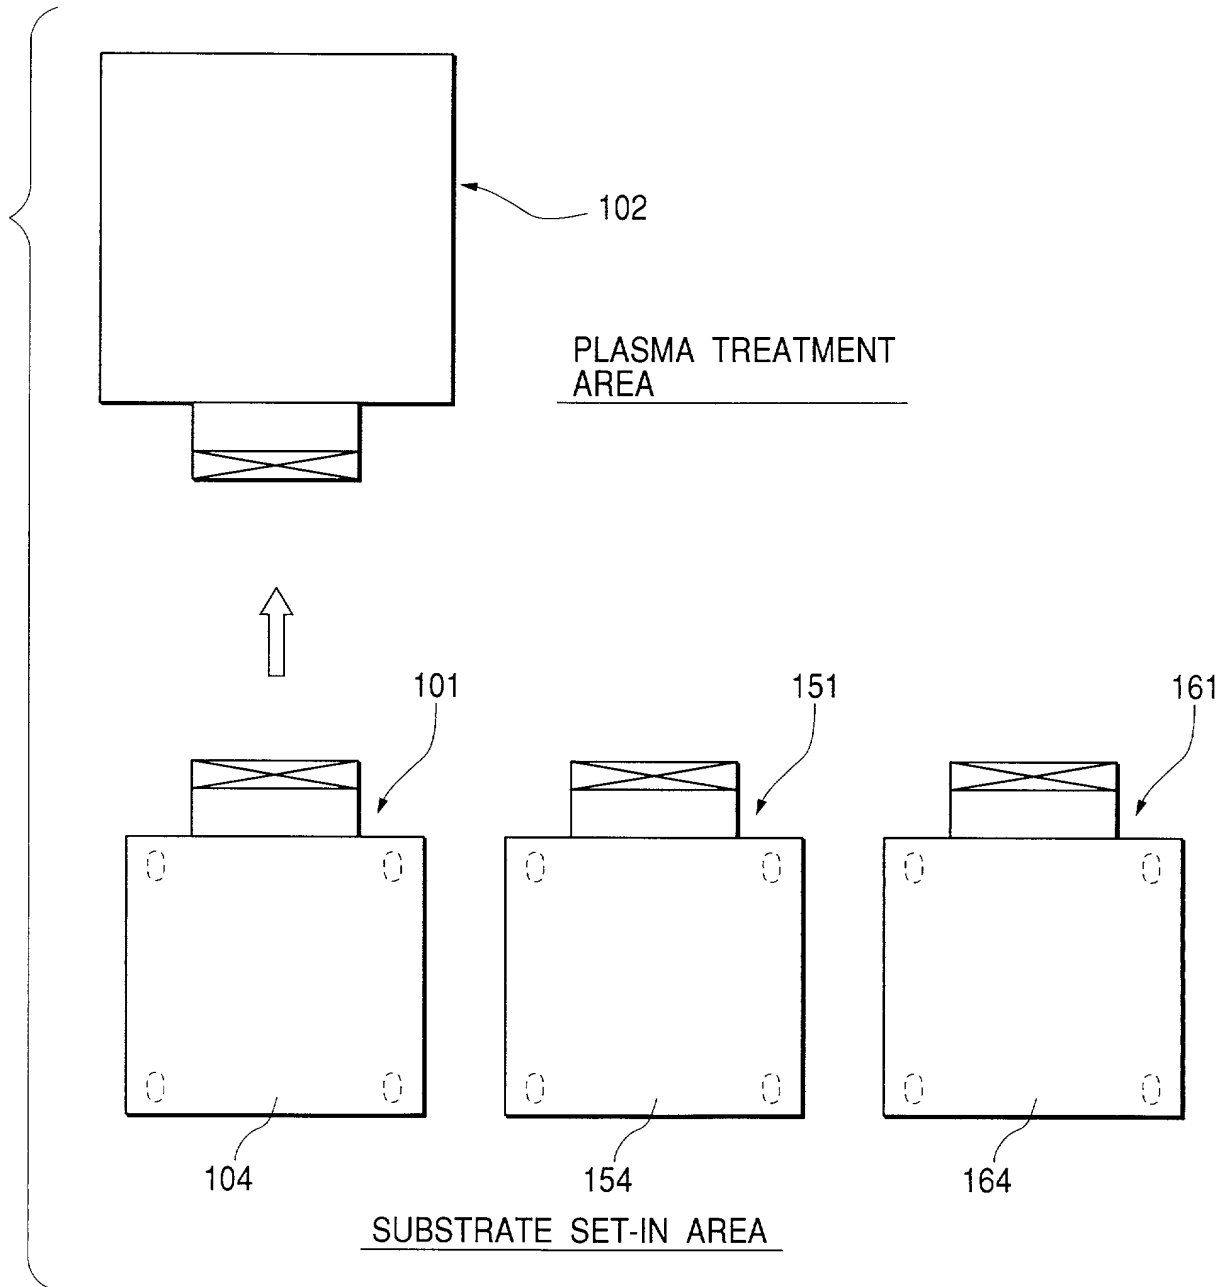


FIG. 2

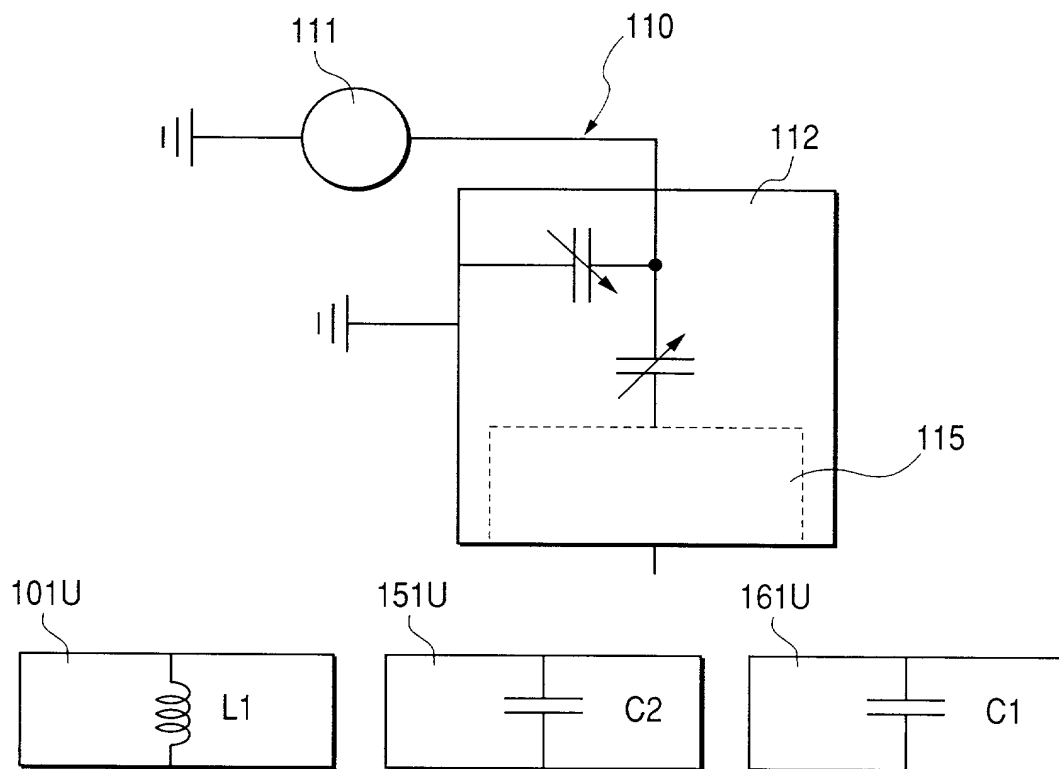
FIG. 3

FIG. 4

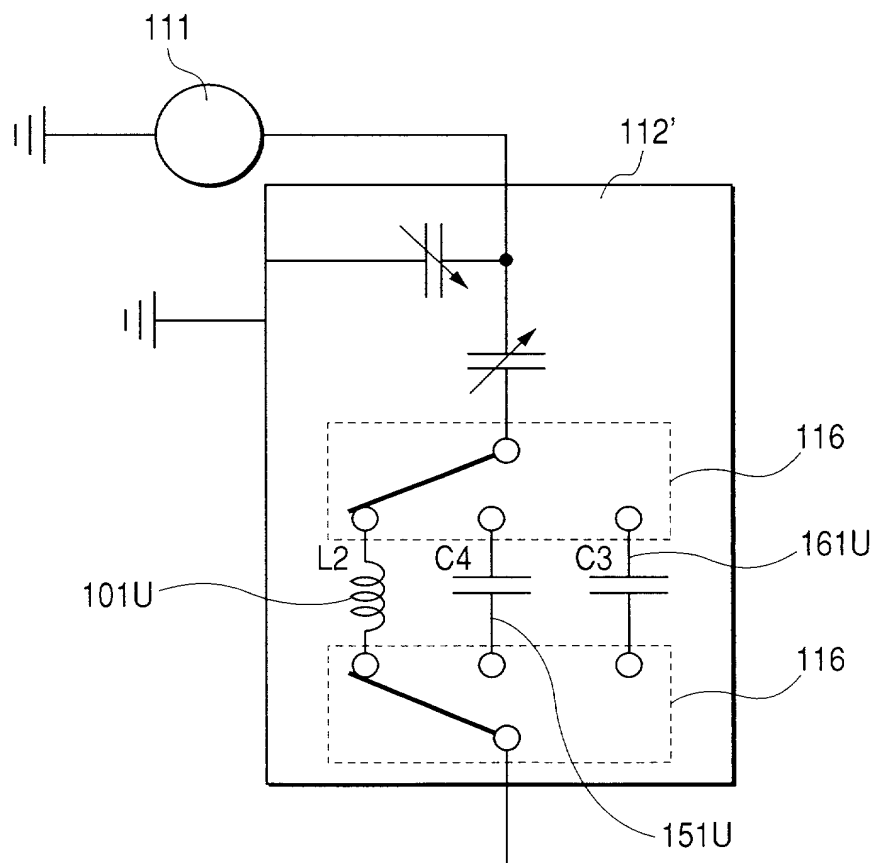


FIG. 5

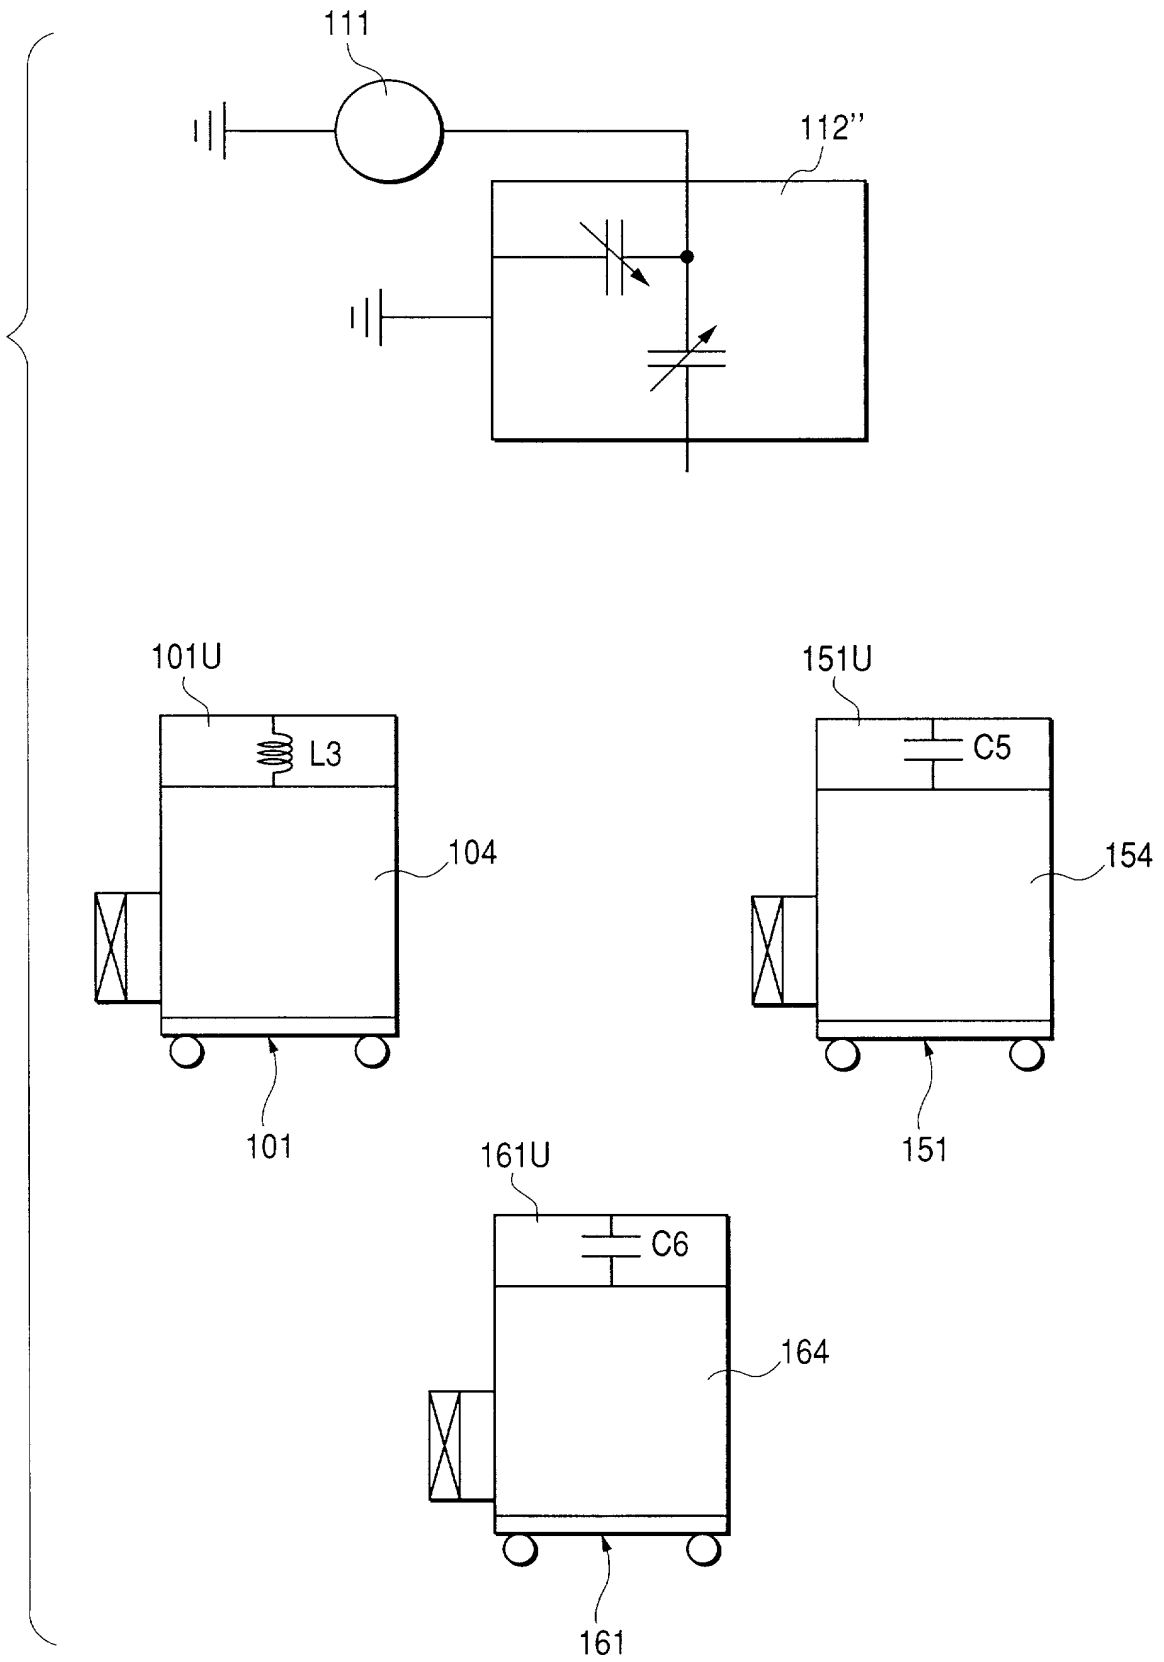


FIG. 6A

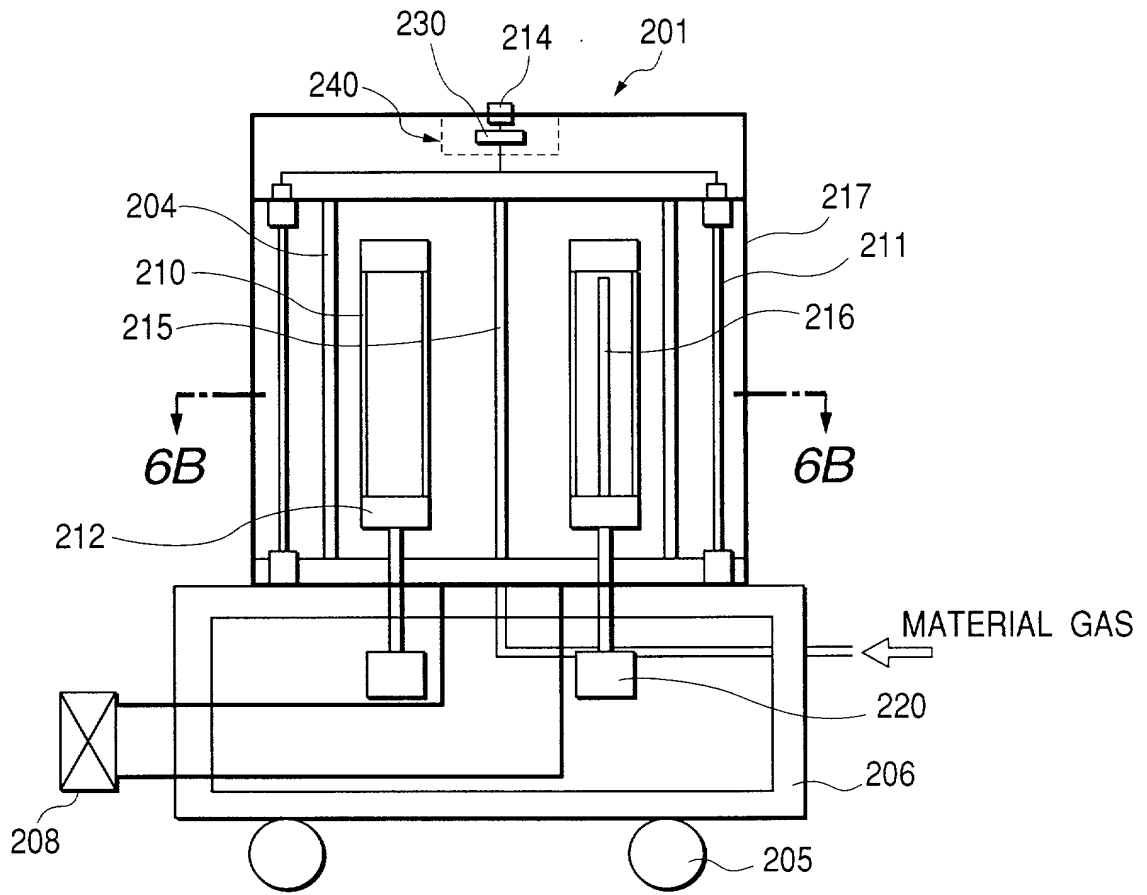


FIG. 6B

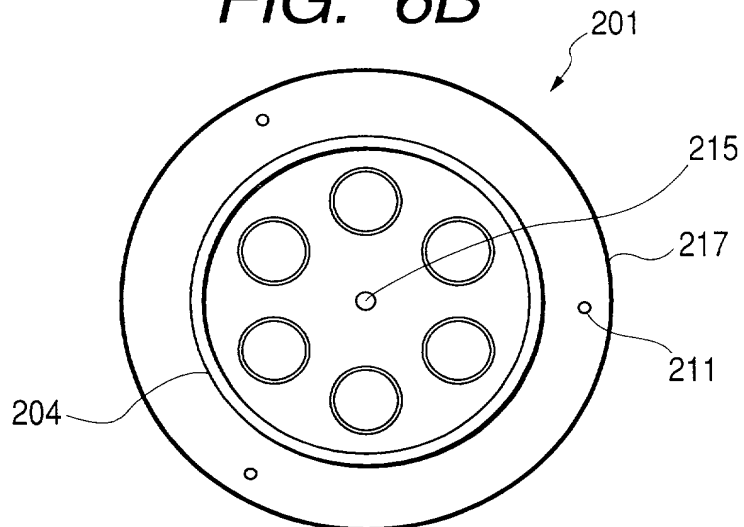


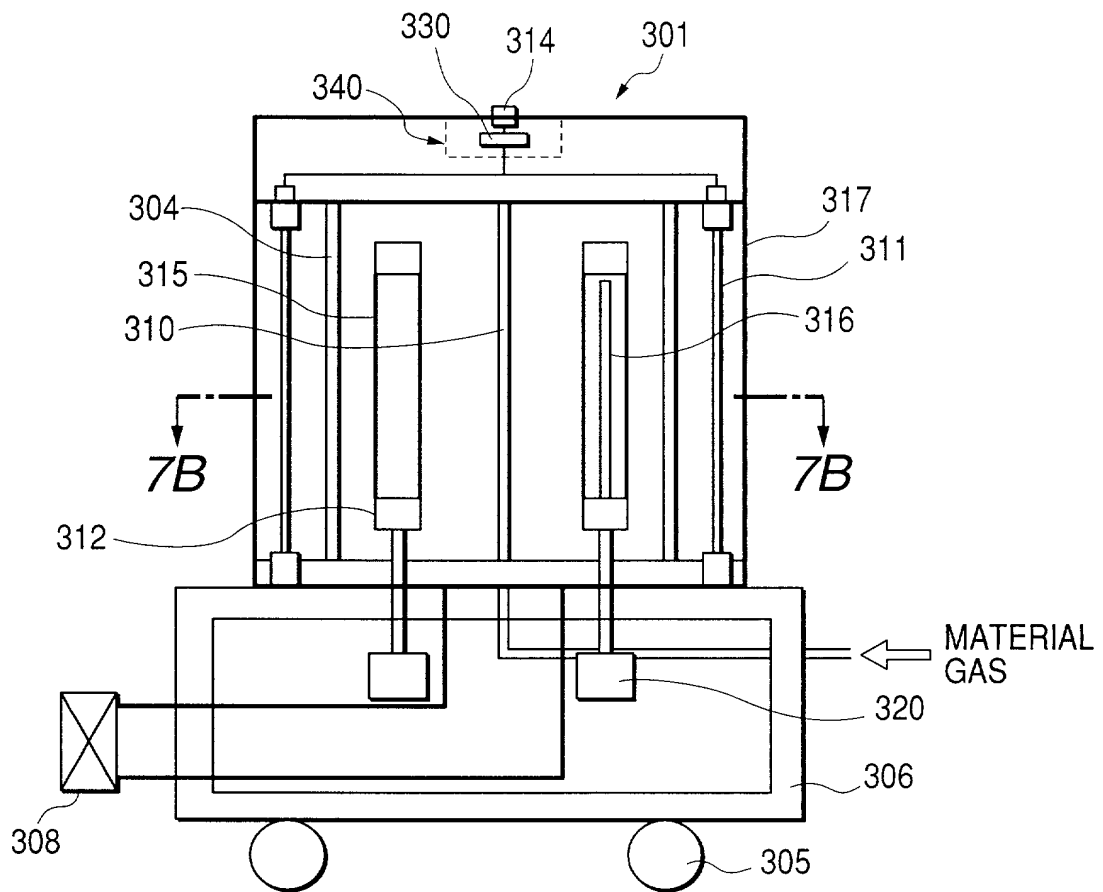
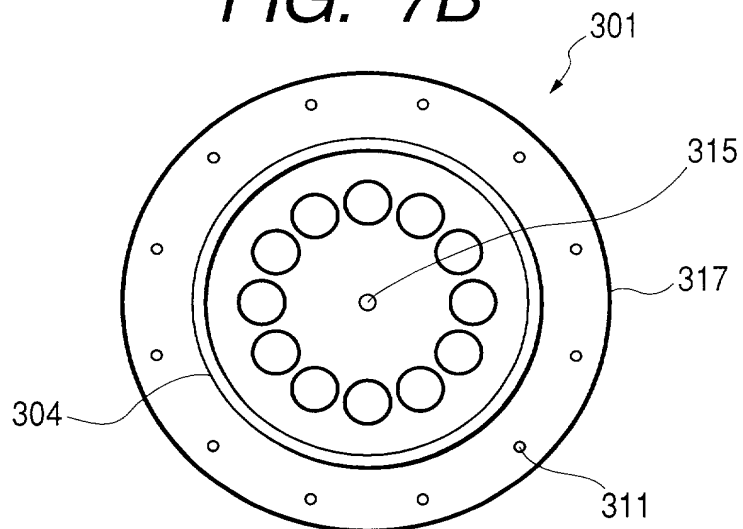
FIG. 7A**FIG. 7B**

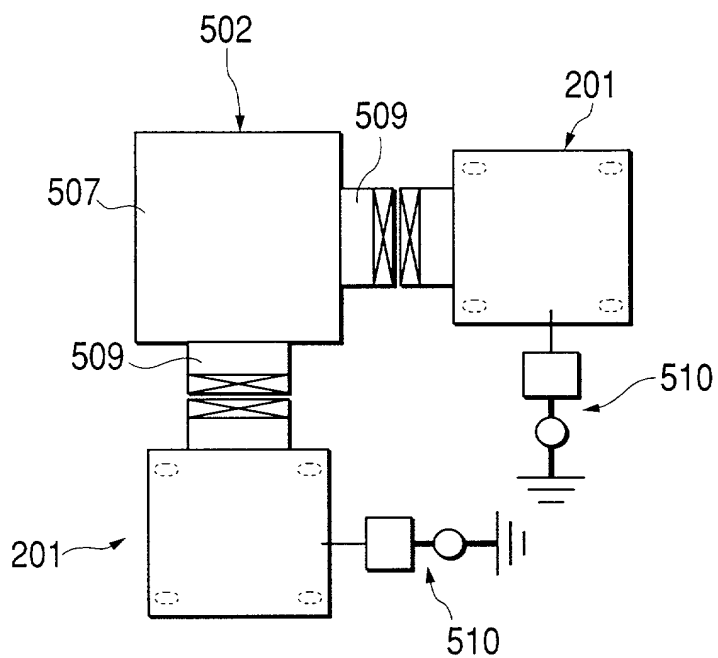
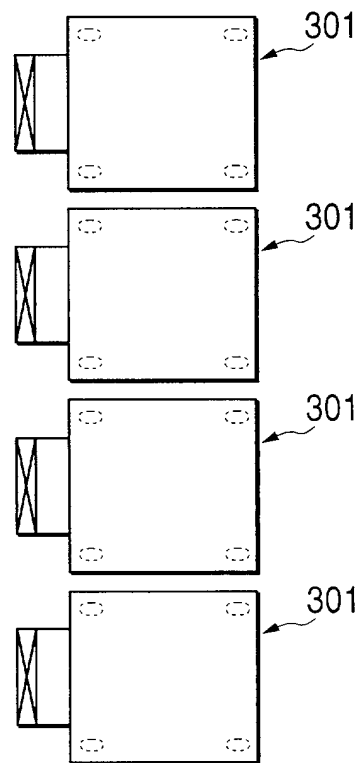
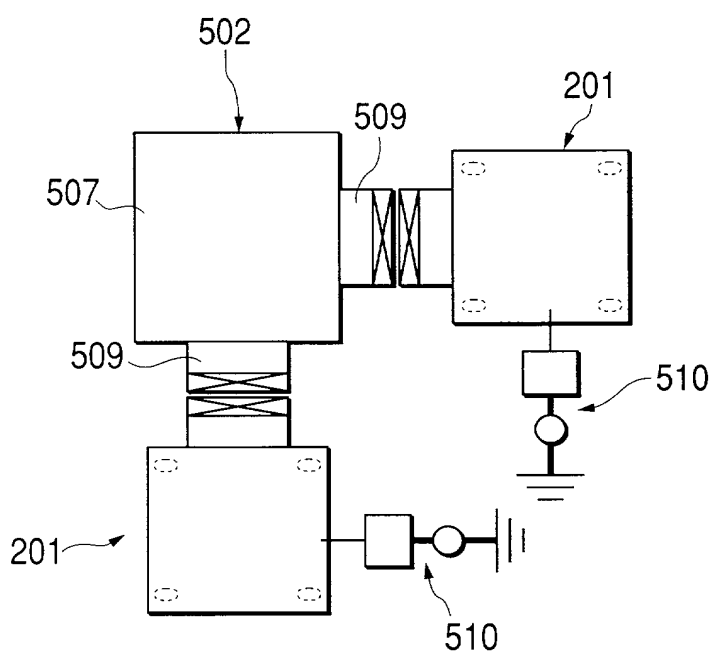
FIG. 8PLASMA TREATMENT AREAPLASMA TREATMENT AREA

FIG. 9

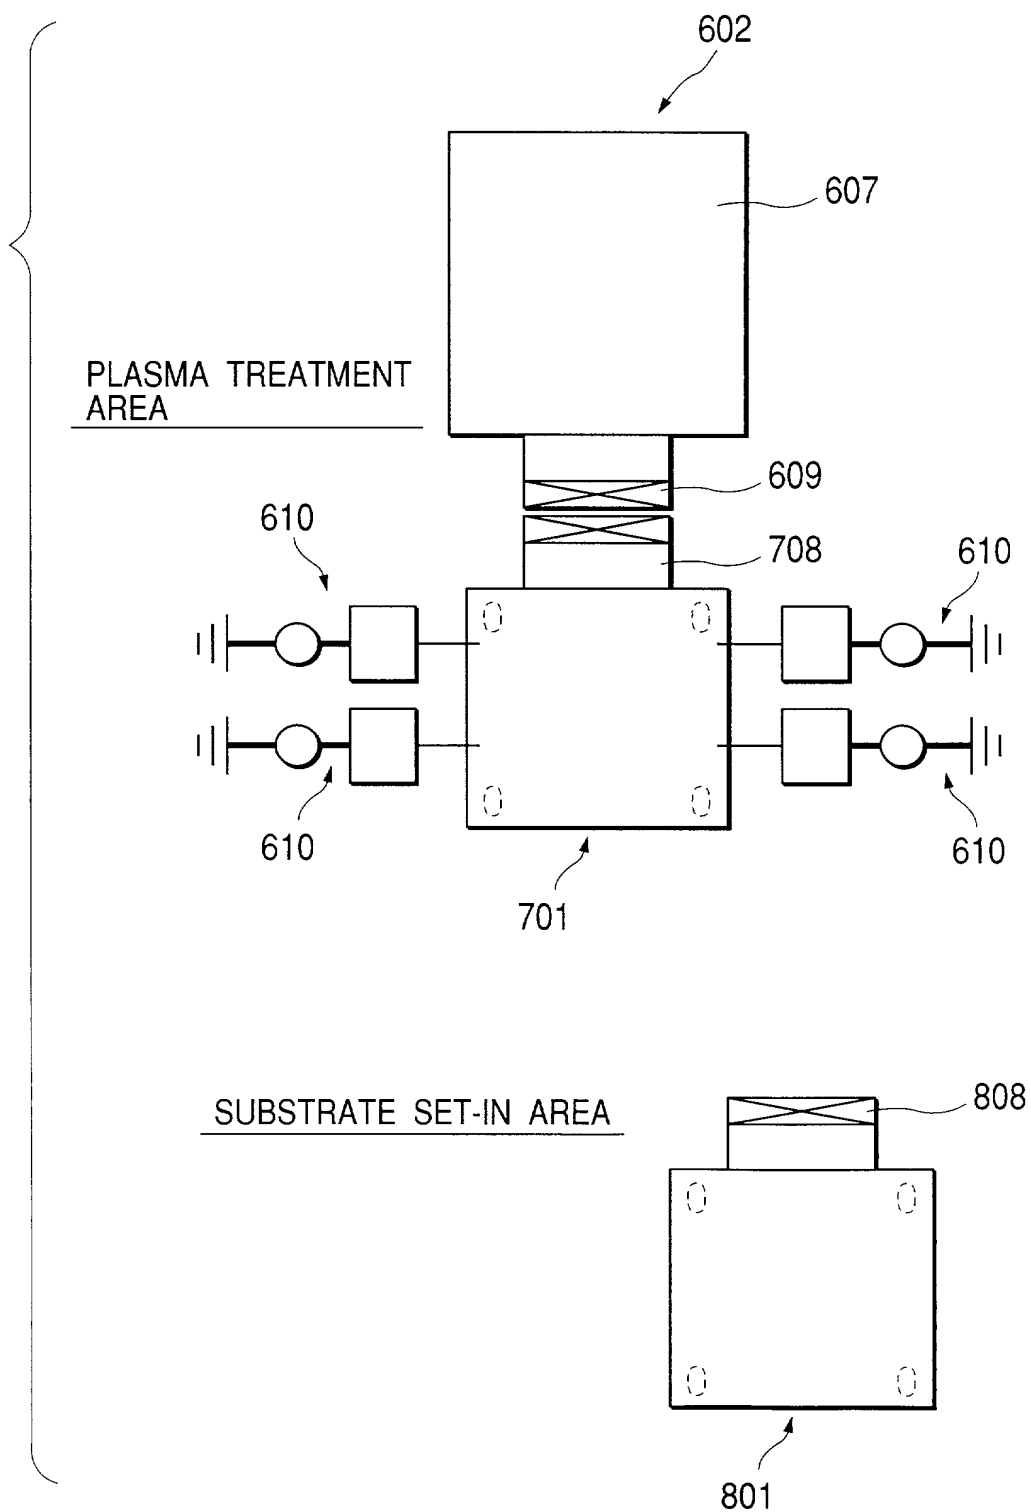


FIG. 10A

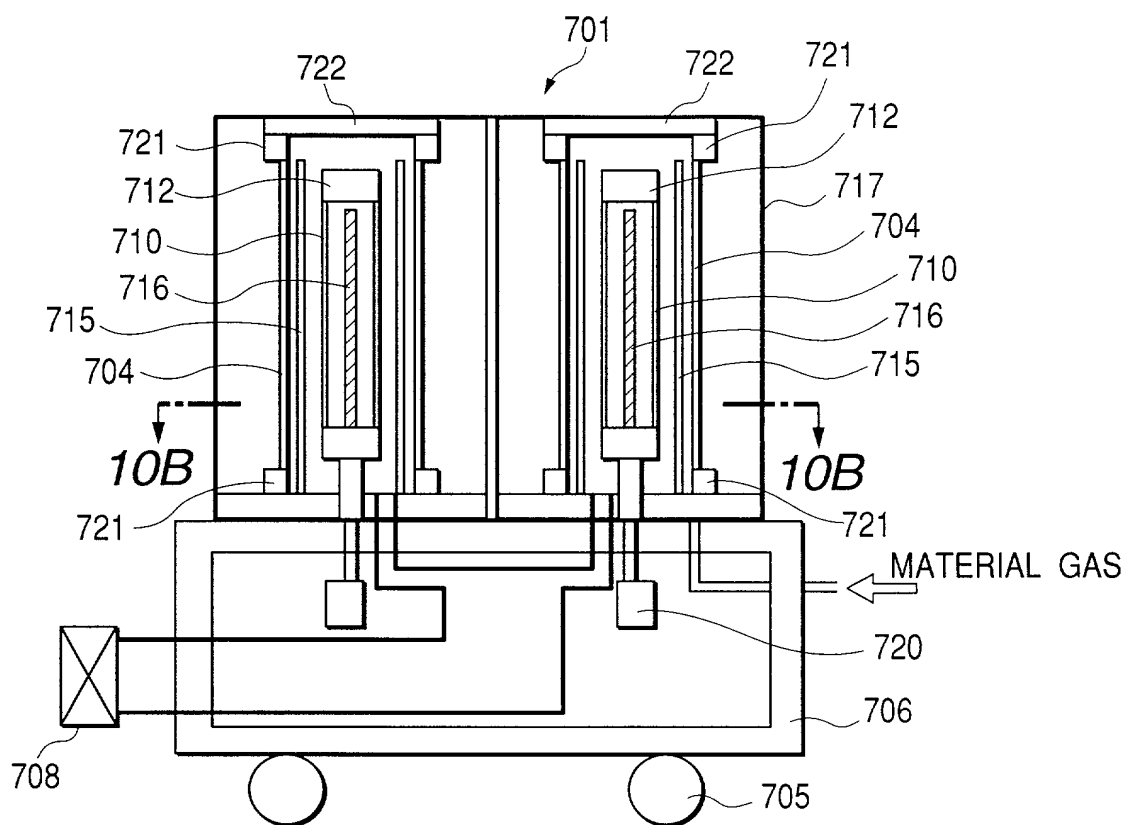


FIG. 10B

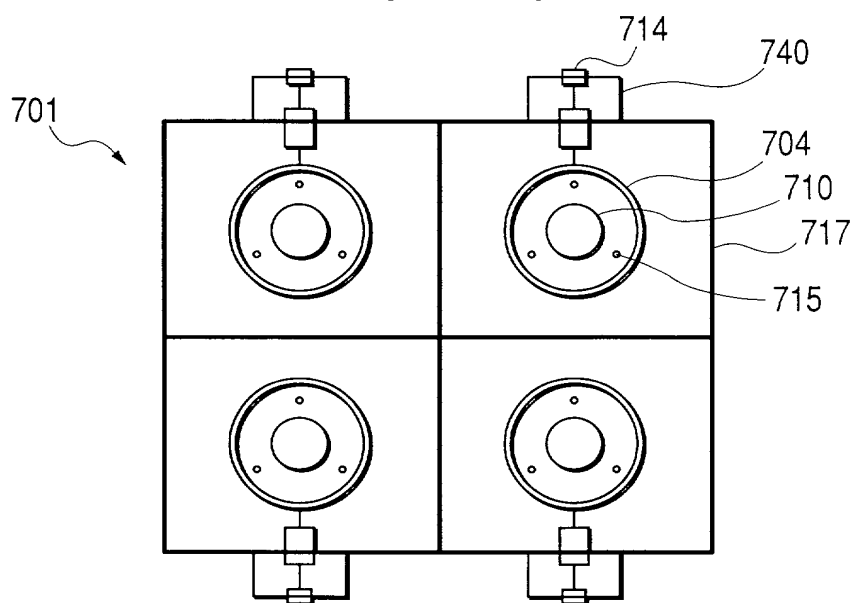


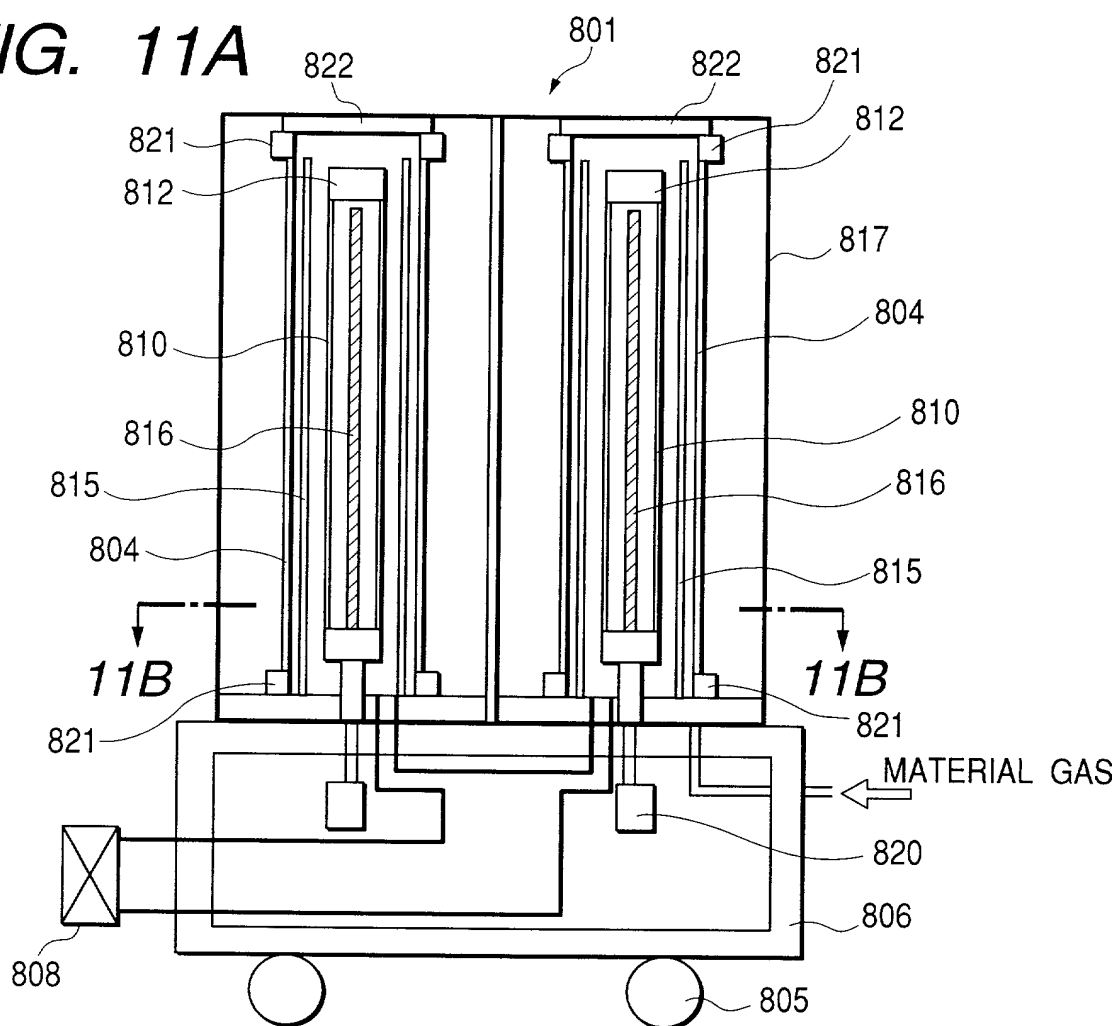
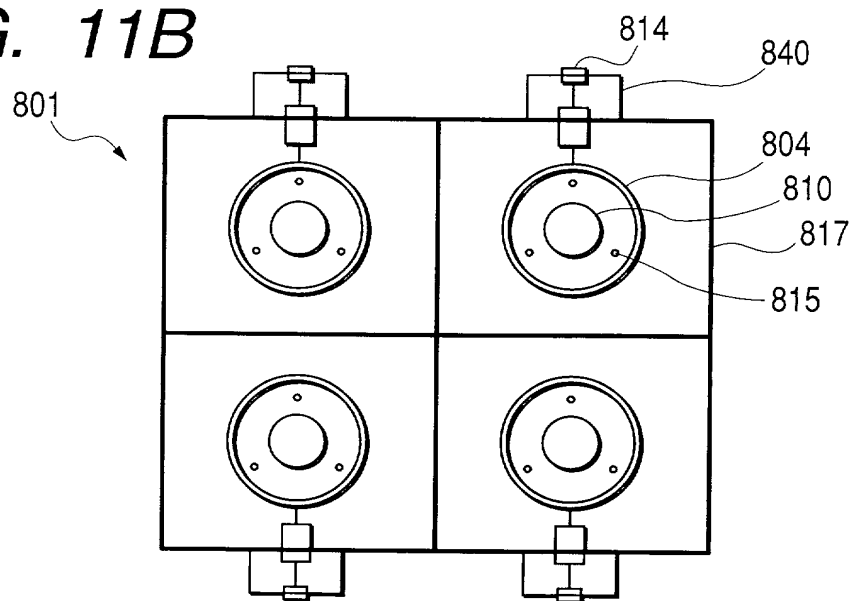
FIG. 11A**FIG. 11B**

FIG. 12A

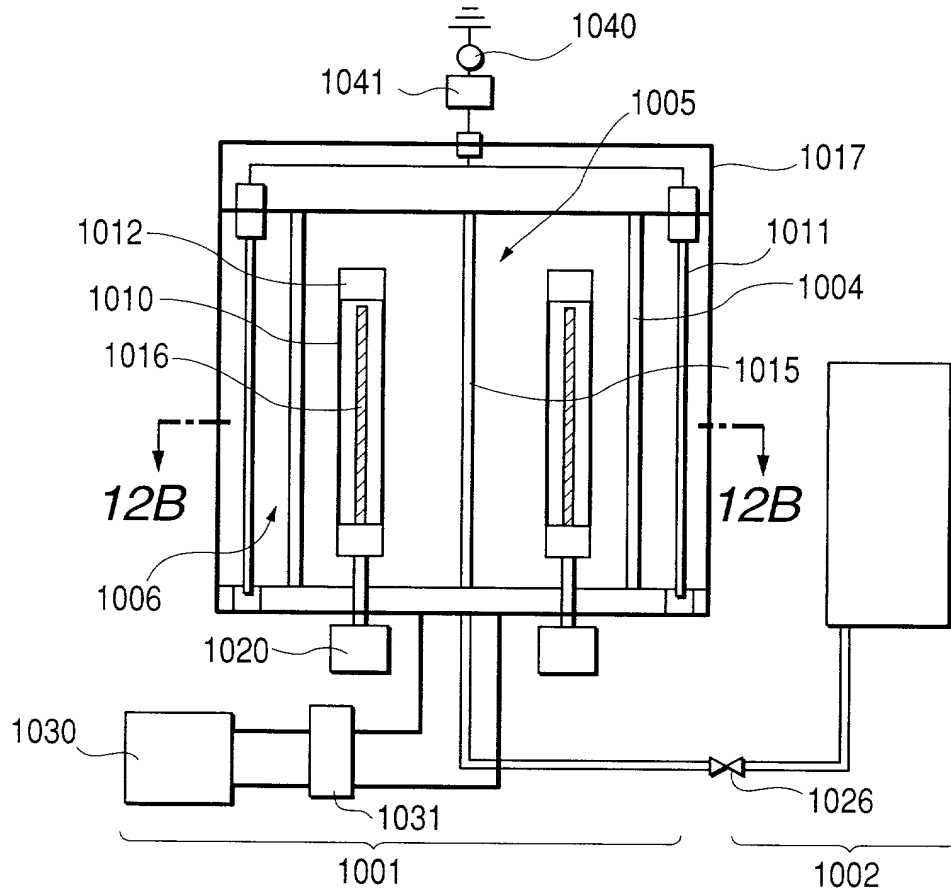


FIG. 12B

